


Designed for Trans Oral Robotic Surgery (TORS), Laser, Mini-invasive & Endoscopic procedures in Tongue base, Hypopharynx, Oropharynx and Larynx.

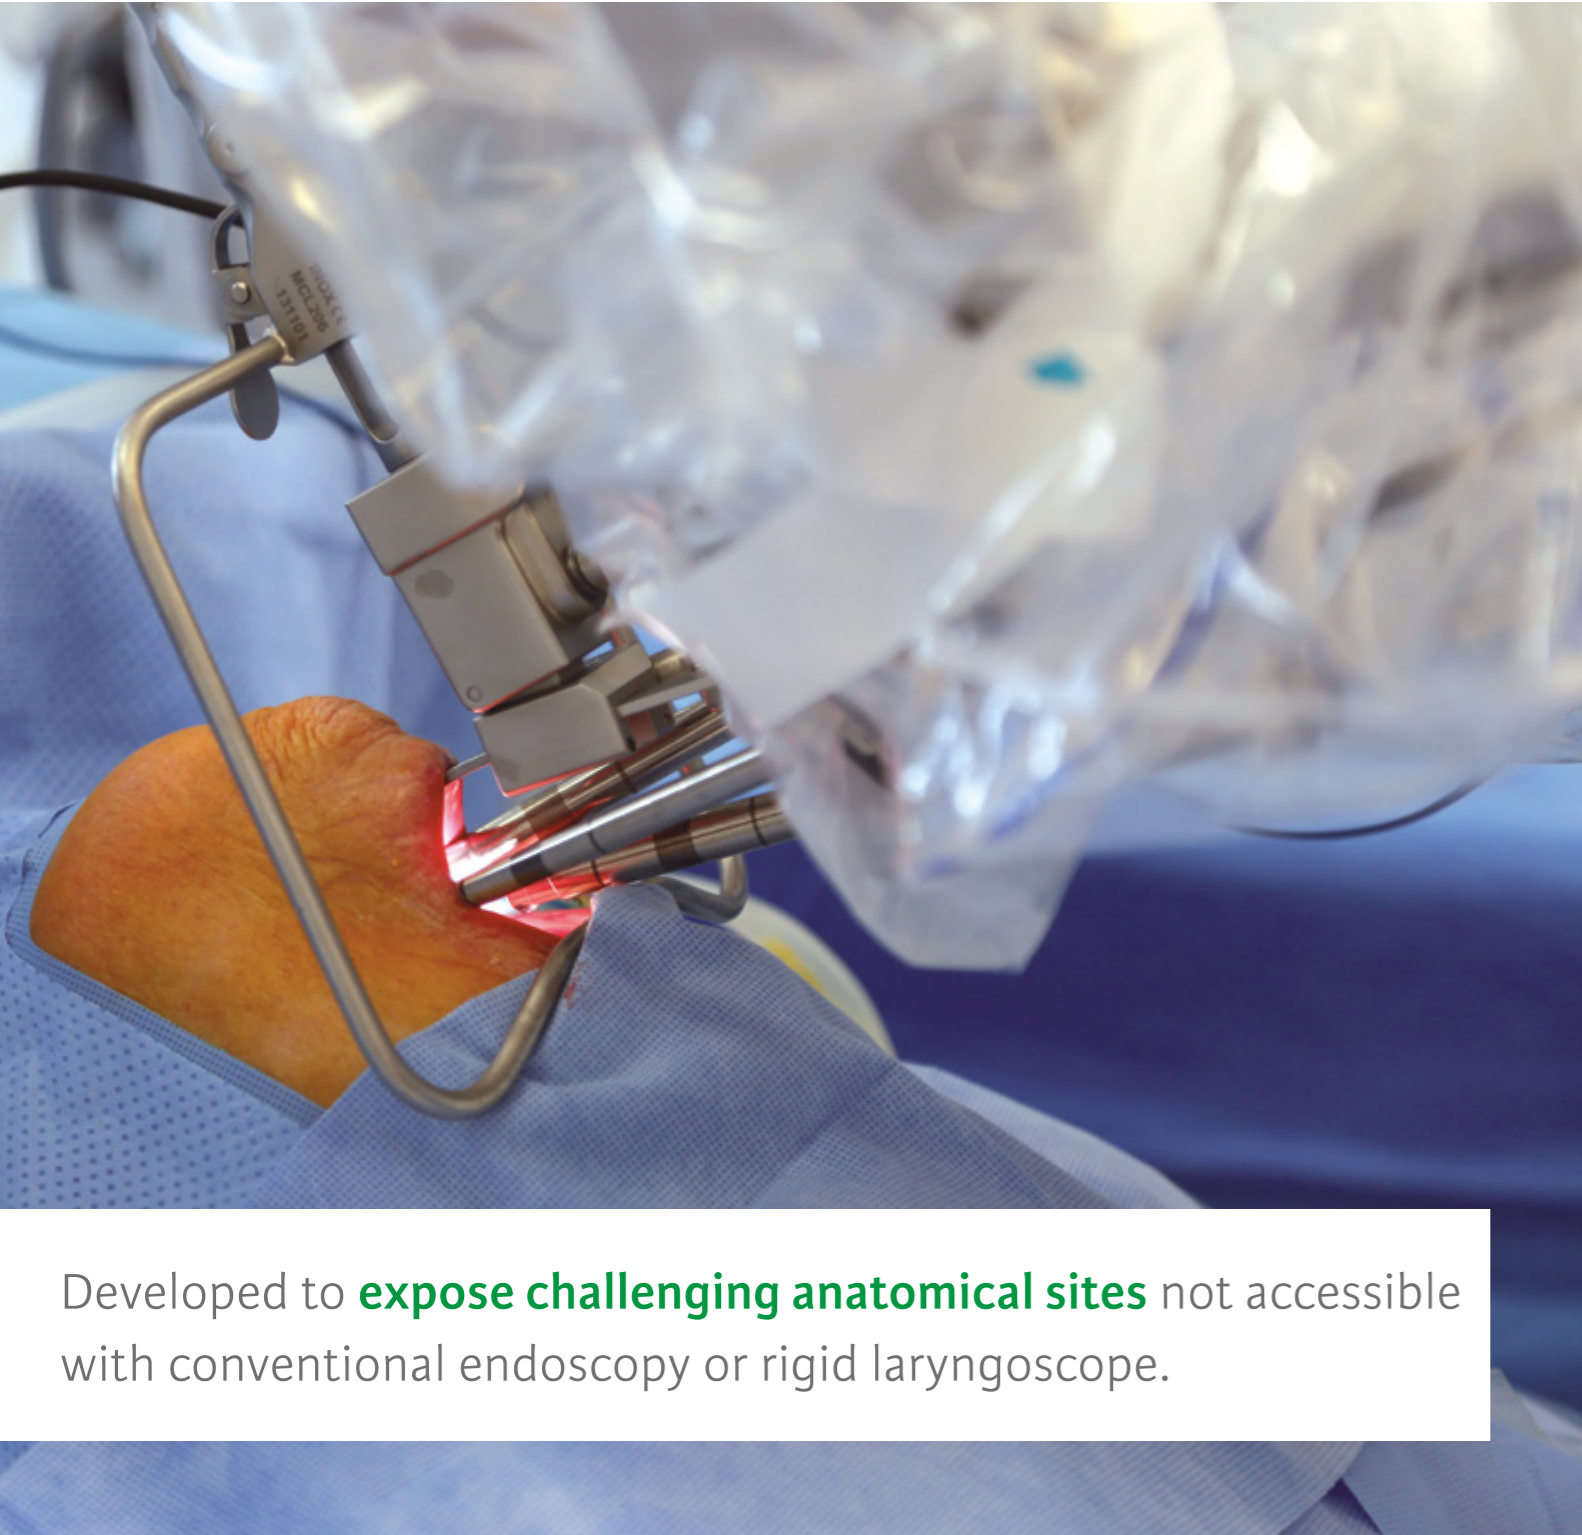

Developed to **expose challenging anatomical sites** not accessible with conventional endoscopy or rigid laryngoscope.

Integra® MicroFrance® MCL206 includes\*:

Reference	Descriptions
MCL206C	Mouth-gag frame
7802P	Dental mouth guard (pack 2)
MCL206A1	Blade 35x120mm Fenestrated
MCL206A2	Blade 35x120mm
MCL206A3	Blade 35x110mm
MCL206A4	Blade 40x85mm
MCL206A5	Blade 35x65mm
MCL206K	Tightening key
MCL206P	Angled adaptor for the suspension with the chest holder (MCL76 + MCL 35)

\*any of the above components may be ordered separately

Optional Accessories:

Reference	Descriptions
MCL206A6	Blade 20x140mm
MCL206A7	Blade 23x180mm
7960T40 <sup>(D)</sup>	Dental mouth guard – single use, sterile (pack 40)
MCL76	Declutching arm holder
MCL35	Plate for MCL76
MCL89-1	Suction tube
MCL100	Blunt eyes suction tube
MCL89-2	Light fiber
MCL38N <sup>(D)</sup>	Cold light cable 2200mm
MCL170 <sup>(D)</sup>	Wolf adapters for light fiber
MCL171 <sup>(D)</sup>	
MCL173 <sup>(D)</sup>	Storz adapters for light fiber
MCL174 <sup>(D)</sup>	
MCL197 <sup>(D)</sup>	Olympus adapter for light fiber

<sup>(D)</sup> Products distributed by Integra MicroFrance SAS (France)

#### INDICATIONS FOR USE

Manual surgical instruments are intended for use in a wide variety of surgical procedures including various laparoscopic and endoscopic procedures. The instruments are intended to scrape, cut, grasp, hold, remove, or manipulate tissue or structures. Wormald Vascular Clamps are indicated for use for temporary or partial occlusion of blood vessels during surgical procedures.

#### CONTRAINDICATIONS

None known.

Availability of these products might vary from a given country or region to another, as a result of specific local regulatory approval or clearance requirements for sale in such country or region.

- Non contractual document. The manufacturer reserves the right, without prior notice, to modify the products in order to improve their quality.
  - Warning: Applicable laws restrict these products to sale by or on the order of a physician.
  - Consult product labels and inserts for any indications, contraindications, hazards, warnings, precautions, and instructions for use.
- Products mentioned in this document are CE class I and IIa devices. Contact Integra should you need any additional information on devices classification. All the medical devices mentioned in this document are CE marked according to European council directive 93/42/EEC on medical devices and its relatives, unless specifically identified as "NOT CE MARKED".

For more information or to place an order, please contact:

**Sales & Marketing EMEA**  
 Integra LifeSciences Services (France) SAS  
 Immeuble Séquoia 2 ▪ 97 allée Alexandre Borodine  
 Parc technologique de la Porte des Alpes  
 69800 Saint Priest ▪ FRANCE  
 Phone: +33 (0)4 37 47 59 00 ▪ Fax: +33 (0)4 37 47 59 99  
 integralife.eu



**Manufacturer:**  
 Integra MicroFrance SAS (France)  
 Le Pavillon ▪ 03160 Saint Aubin le Monial  
 France



Sunoptic Technologies, LLC  
 6018 Bowdendale Avenue ▪ Jacksonville  
 FL 32216 USA



RMS – UK Limited  
 28 Trinity road ▪ Nailsea  
 Somerset ▪ BS48 4NU ▪ UK



Directa AB  
 19427 Upplands ▪ Vasby  
 Sweden

#### Integra Contact - Questions, Information & Product Ordering

International: +33 (0) 437 47 59 50 ▪ +33 (0) 437 47 59 25 (Fax) ▪ csemea@integralife.com  
 France: +33 (0) 437 47 59 10 ▪ +33 (0) 437 47 59 29 (Fax) ▪ custsvcf@integralife.com  
 United Kingdom: +44 (0) 1264 345 780 ▪ +44 (0) 1264 363 782 (Fax) ▪ custsvcs.uk@integralife.com  
 Italy: +39 (0)2 577 89 21 ▪ +39 (0)2 575 113 71 (Fax) ▪ custsvcitaly@integralife.com  
 Benelux: +32 (0)2 257 4130 ▪ +32 (0)2 253 2466 (Fax) ▪ custsvcbenelux@integralife.com

Integra and the Integra logo are registered trademarks of Integra LifeSciences Corporation in the United States and/or other countries. MicroFrance is a registered trademark of Integra LifeSciences Corporation or its subsidiaries in the United States and/or other countries. Document for use in Europe, Middle-East and Africa only. ©2017 Integra LifeSciences Corporation. All rights reserved. Last revision date: 10/2017. 0679141-3-EN



Mouth-gag for pharyngolarynx exposure in trans-oral surgery

**Integra® MicroFrance®**


**Morinière Mouth-gag**

For ambitious aerodigestive surgical site exposure




### An ergonomic system for robotic surgery:

Wide exposure for difficult lesions access with multiple surgical instruments

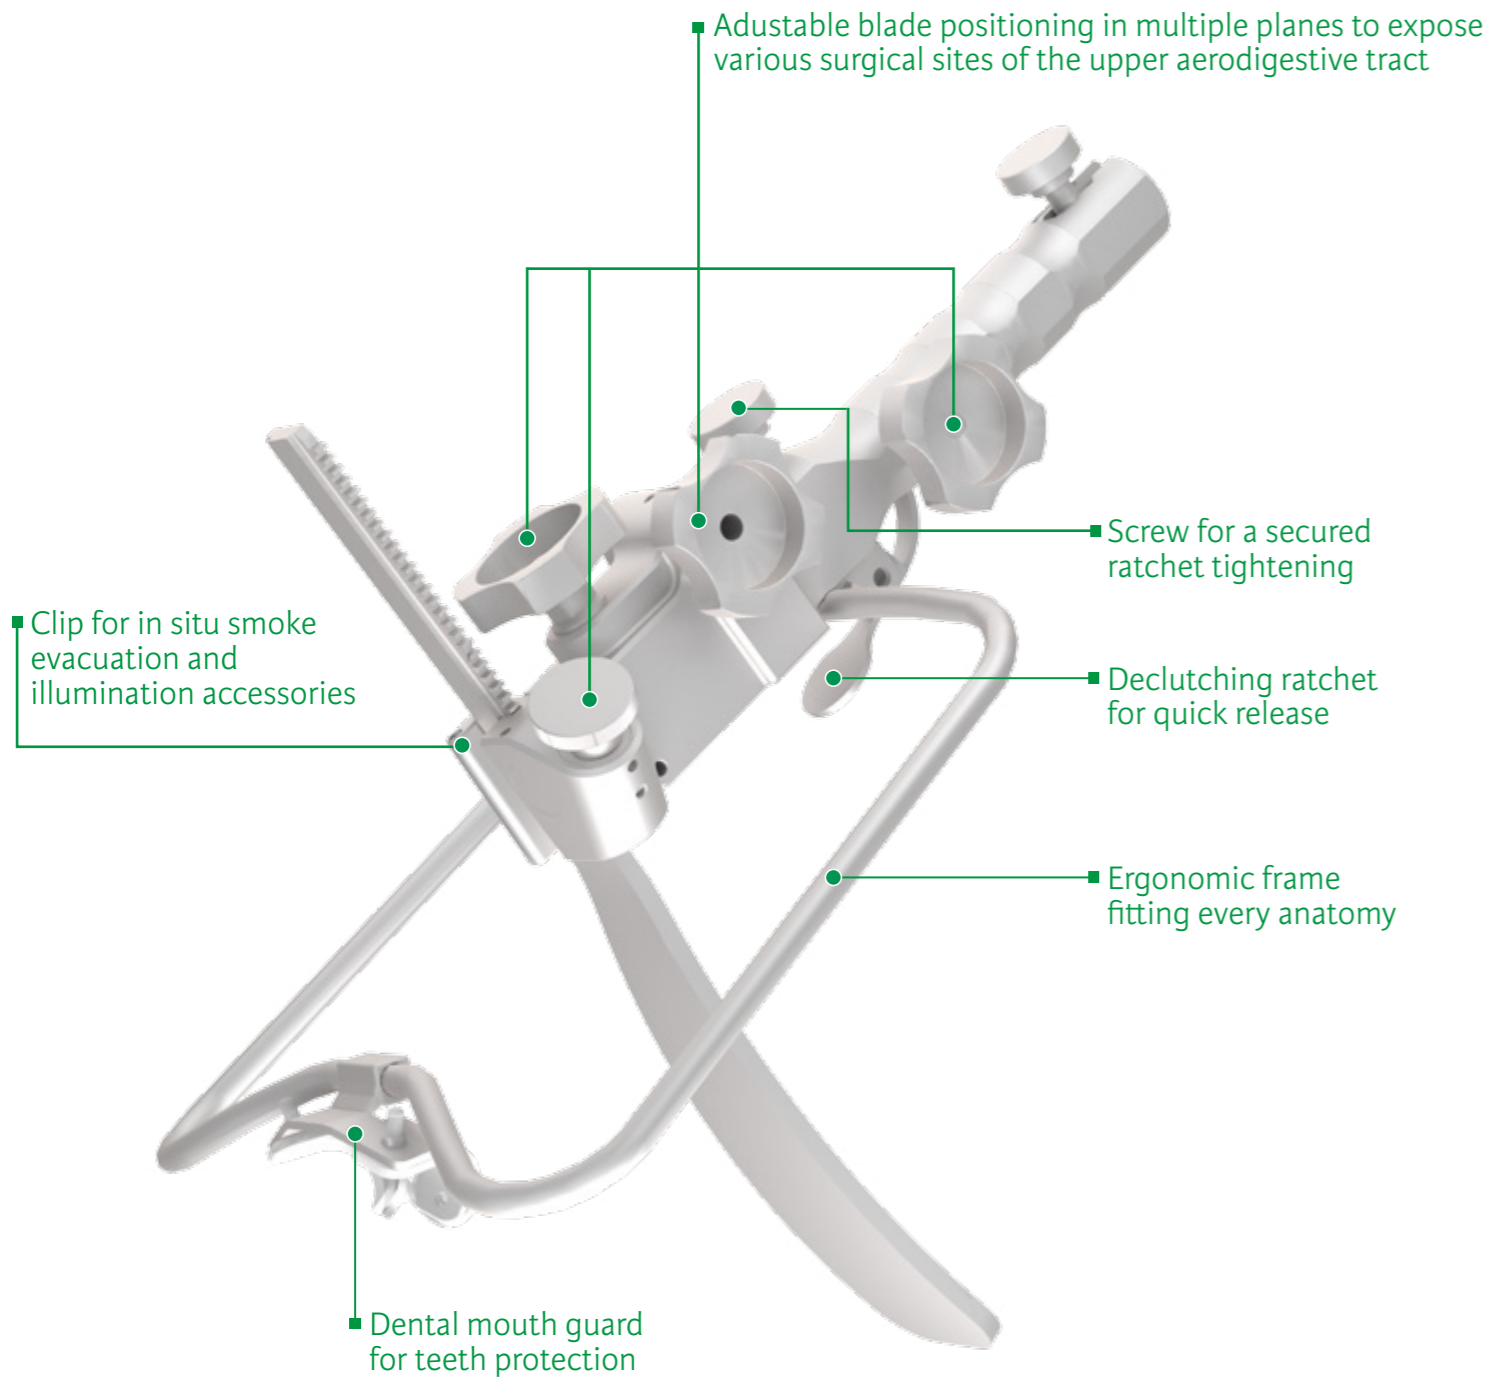

### Setting the adequate exposure during intervention:

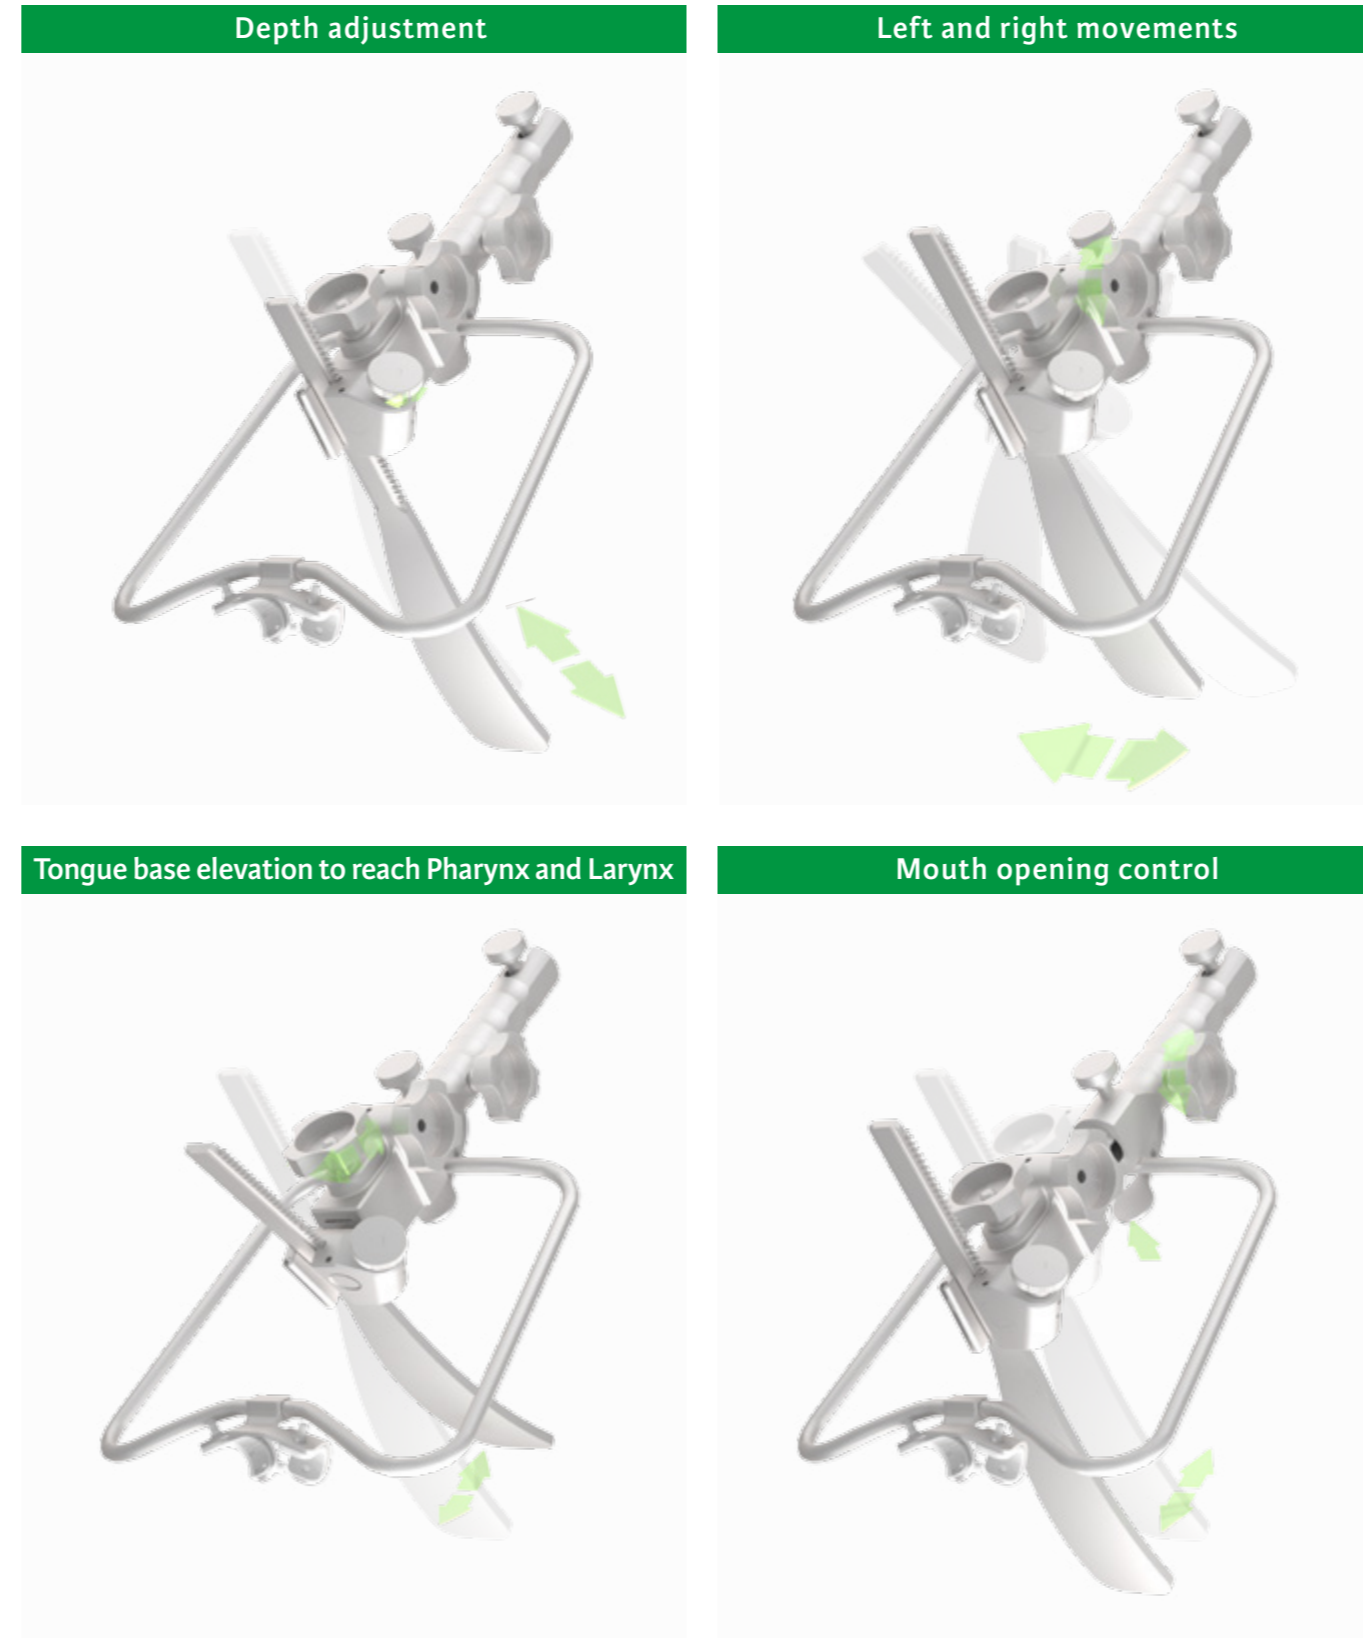

### Multiple blades design for specific area and various anatomic exposure:

- 3 blades for Hypopharynx & Pharynx access
- 2 smaller blades for Oropharynx access



- 1 blade for Larynx access\*



- 1 blade for Zenker's Diverticulum access\*



\* equipped with a guide for light fiber or smoke suction placement

### Accessories:

